


Spectrum Point Pick Report

07/09/2025 04:49:28 PM

Data Set: A crassicauda090725-sol - RawData-003

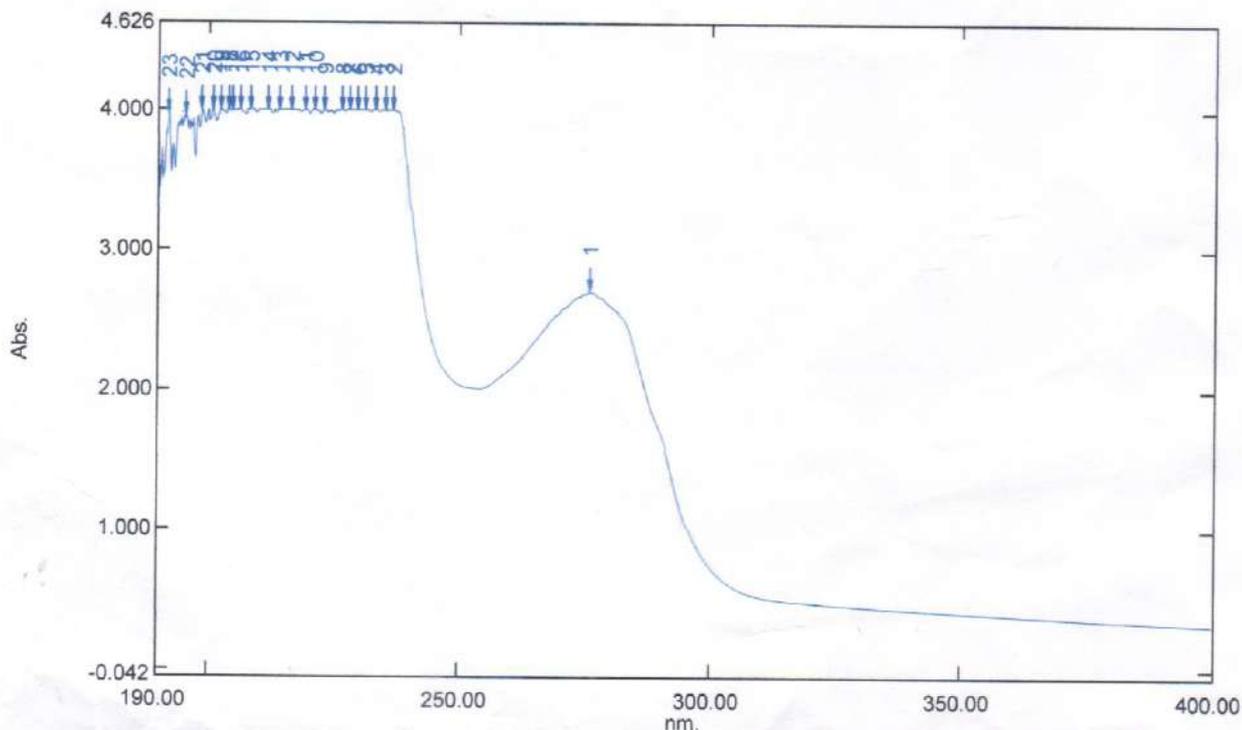

[Measurement Properties]
 Wavelength Range (nm.): 190.00 to 400.00
 Scan Speed: Fast
 Sampling Interval: 0.1
 Auto Sampling Interval: Disabled
 Scan Mode: Repeat

No.	Wavelength	Absorbance	Description
1	275.90	2.701	
2			

[Instrument Properties]
 Instrument Type: UV-1900 Series
 Measuring Mode: Absorbance
 Slit Width: 1.0 nm
 Light Source Change Wavelength: 340.8 nm
 S/R Exchange: Normal

[Attachment Properties]
 Attachment: None

[Operation]
 Threshold: 0.0010000
 Points: 4
 InterPolate: Disabled
 Average: Disabled

[Sample Preparation Properties]
 Weight:
 Volume:
 Dilution:
 Path Length:
 Additional Information: